

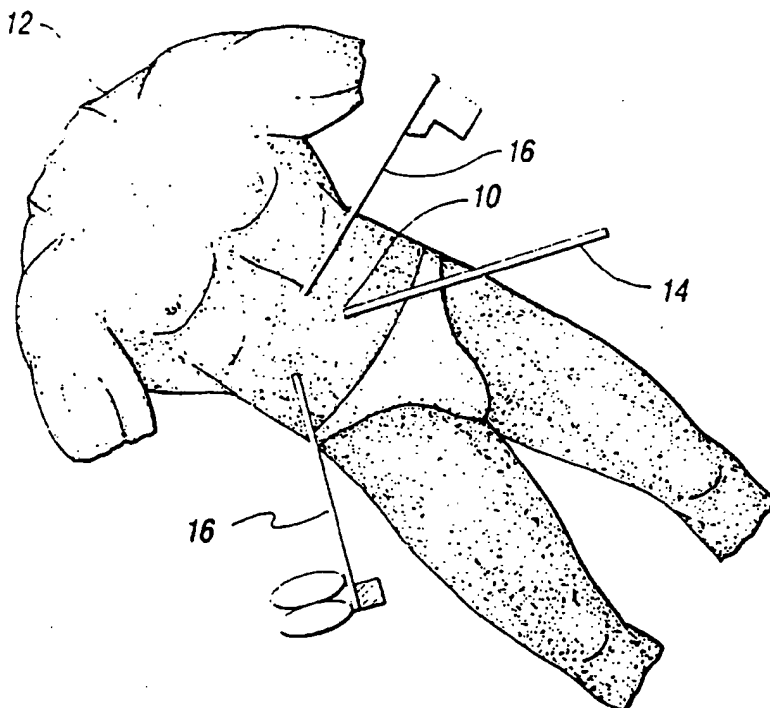
**PCT**WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification <sup>6</sup> :</b> <b>G09B 23/28, A61B 1/00, 19/00</b>	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 95/02233</b> <b>(43) International Publication Date:</b> 19 January 1995 (19.01.95)
<b>(21) International Application Number:</b> PCT/US94/07218 <b>(22) International Filing Date:</b> 27 June 1994 (27.06.94) <b>(30) Priority Data:</b> 087,653                      6 July 1993 (06.07.93)                      US <b>(71) Applicant:</b> CYBERNET SYSTEMS CORPORATION [US/US]; Suite B-101, 1919 Green Road, Ann Arbor, MI 48105 (US). <b>(72) Inventors:</b> JACOBUS, Charles, J.; 820 Heatherway, Ann Arbor, MI 48104 (US). GRIFFIN, Jennifer, Lynn; #203, 1895 Pointe Crossing, Ann Arbor, MI 48105 (US). <b>(74) Agent:</b> SYROWIK, David, R.; Brooks & Kushman, 22nd floor, 1000 Town Center, Southfield, MI 48075 (US).		<b>(81) Designated States:</b> AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  <b>Published</b> <i>With international search report.</i>

**(54) Title:** METHOD AND SYSTEM FOR SIMULATING MEDICAL PROCEDURES INCLUDING VIRTUAL REALITY AND CONTROL METHOD AND SYSTEM FOR USE THEREIN**(57) Abstract**

During an actual medical procedure, the actions of a medical instrument (16) are measured and recorded. These actions are generated on a member representative of the medical instrument to simulate the actual medical procedure. Forces acting upon the medical instrument (16) are sensed and simulated in the member using a force/tactile reflecting mechanism. The preferred embodiment uses virtual reality technology including image processing, three-dimensional graphics and display methods, simulated force/tactile reflection, head/hand movement, position sensing, and sound generation to provide an accurate simulation of endoscopic medical procedures.



**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

**METHOD AND SYSTEM FOR  
SIMULATING MEDICAL PROCEDURES  
INCLUDING VIRTUAL REALITY AND CONTROL  
METHOD AND SYSTEM FOR USE THEREIN**

5                    **Cross-Reference To Related Application**

                  This application is a continuation-in-part of  
copending U.S. application Serial No. 984,324, filed  
December 2, 1992.

**Technical Field**

10                    This invention relates to methods and systems  
for simulating medical procedures for training and for  
remote control.

**Background Art**

15                    Laparoscopic surgery, a specific application  
of endoscopic surgery, is performed by:

                  (1) making several small openings into the  
peritoneal cavity 10 of the body 12 as shown in Figure  
1;

20                    (2) insufflating with an inert gas, CO<sub>2</sub>  
(providing medium for adequate anatomical inspection);

                  (3) inserting a viewing scope 14 (laparo-  
scope) into one opening 10;

25                    (4) inserting other surgical instruments 16  
into the other openings (i.e. staplers, cutting/cauter-  
izing instruments, etc.); and

                  (5) maneuvering and manipulating these  
instruments 16 on the basis of tactile feel and the

-2-

visual information of the surgical site from the inserted viewing scope 14 (usually displayed on a TV monitor).

Because the feel of the instruments 16 and the imagery of the surgical site is restricted to a small local area which is not directly visible, surgeons must train extensively (usually on animals) prior to performing human procedures. This type of surgery is still very much an art rather than science.

Endoscopic and laparoscopic intervention is being fervently applied to procedures (such as cholecystectomies, hernia repair, nephrectomies, appendectomies, and numerous gynecological procedures) being praised for fast patient recovery time and decreased hospital and surgery costs. As new applications emerge, training will play a crucial role in technological adoption. A need exists for a training device which will facilitate the transition from more traditional open procedures to endoscopic procedures by fostering the surgical skill necessary for the execution of efficient and complication-free procedures.

U.S. Patent No. 5,149,270, issued to McKeown, discloses an apparatus for practicing endoscopic surgical procedures. The apparatus has a cavity in which an object simulating a human organ is mounted for performing a practice procedure. The cavity is closeable to outside view, thereby forcing the individual practicing the procedure to use and manipulate the instruments relying only upon a viewing scope in an attempt to mimic the actual diagnostic and operating conditions. This configuration, by relying upon physical linkages and

-3-

organ materials, lacks the versatility, robustness, and repeatability of a programmable simulation device.

International PCT application No. PCT/US92/02186, published 1 October 1992, discloses an automated surgical system and apparatus. An endoscopic instrument and a viewing scope are controlled remotely via a control mechanism in communication with the surgical instruments over a telecommunications link. This device, while directed toward the remote control of surgical instruments, does not address the necessity of force feedback for giving the remote user the feel of actual surgical procedures. Further, the device is directed toward remotely performing actual surgical procedures rather than simulated surgical procedures for the purposes of training.

### **Summary of the Invention**

It is an object of the above invention to provide a method and system for simulating actual medical procedures.

20 A further object of the above invention is to provide a method for providing a virtual reality in response to a position and orientation of a member representative of a medical instrument.

25 Moreover, an object of the above invention is to provide a method and system for controlling a medical instrument.

-4-

An additional object of the above invention is to provide a four-axis controller for a medical instrument.

5 In carrying out the above objects, the present invention provides a method for simulating actual medical procedures which utilize at least one medical instrument. According to the present invention, the actions of the medical instrument are measured during an actual medical procedure. These measured actions of the  
10 medical instrument are generated on a member representative of the medical instrument so as to simulate the actual medical procedure.

In carrying out the above objects, the present invention further provides a system for simulating  
15 actual medical procedures which utilize at least one medical instrument. The system comprises means for measuring the actions of the medical instrument during an actual medical procedure. Means are also provided for generating the measured actions on a member repre-  
20 sentative of the medical instrument whereby the actions of the member simulate the actual medical procedure.

In carrying out the above objects, the present invention also provides a method for providing a virtual reality in response to a position and orientation of a  
25 member representative of a medical instrument. An electrical signal is generated for each of a plurality of degrees of freedom of the member as a function of the position and orientation of the member in three-dimensional space. At least one virtual reality force field  
30 is generated in response to the generated signals. A force signal is generated for each degree of freedom as

-5-

a function of the force field. A force on the member is generated for each force signal, thus providing the virtual reality.

In carrying out the above objects, the present invention additionally provides a method for controlling a medical instrument. The position and orientation of a member representative of the medical instrument is measured. Actions are generated on the medical instrument based upon the measured position and orientation of the member. The forces acting upon the medical instrument are measured. Forces are generated on the member based upon the measured forces acting upon the medical instrument.

In carrying out the above objects, the present invention also provides a system for controlling a medical instrument. The system comprises means for measuring the position and orientation of a member representative of the medical instrument. Means are provided to generate actions on the medical instrument based upon the measured position and orientation of the member. The system further comprises means for measuring the forces acting upon the medical instrument. Means are provided to generate forces on the member based upon the measured forces acting upon the medical instrument.

In carrying out the above objects, the present invention also provides a four-axis controller for a medical instrument. The system comprises a member representative of the medical instrument. A four-axis interface device, which is responsive to the position and orientation of the member, is secured to the member.

-6-

Electrical signals representative of the position and orientation of the member are generated in the four-axis interface device. Means for actuating the medical instrument in response to the electrical signals are included. Means for generating a force field based upon a force induced upon the medical instrument are provided. A force signal for each axis of the interface device is generated by further means, with the actuators responsive to these force signals to provide a force to each axis of the interface device for reflecting a force on the medical instrument to the member.

### **Brief Description Of The Drawings**

FIGURE 1 shows the insertion of a scope and an instrument into a body during a laparoscopic medical procedure;

FIGURE 2 is a block diagram representation of the recording apparatus;

FIGURE 3 depicts the systematic scanning of an anatomical feature to generate a complete imagery record;

FIGURE 4 is a block diagram representation of the virtual reality training/replay apparatus;

FIGURE 5 is a block diagram representation of the incorporation of the recording apparatus with the virtual reality training/replay apparatus;



-7-

FIGURE 6 is a block diagram representation of using the virtual reality replay system to provide a surgeon with preoperative imagery;

FIGURE 7 is a block diagram representation of using the virtual reality system in conjunction with robotic endoscopic medical equipment;

FIGURE 8 is a block diagram representation of the force/tactile subsystem control concept;

FIGURE 9 is a schematic representation of the laparoscopic simulator; and

FIGURE 10 shows the four-axis force reflecting module within an opening in the laparoscopic simulator.

### **Best Mode For Carrying Out The Invention**

Described is a method and an apparatus which uses Virtual Reality Technology including image processing, three dimensional graphics and display methods, simulated force/tactile reflection, programmed stereophonic sound generation, head/hand movement and position sensing to provide an accurate control or simulation of medical procedures, specifically: endoscopic medical procedures including, but not limited to, cholecystectomies, vasectomies, bowel resections, inguinal and bilateral hernia repairs, appendectomies, lymphadenectomies, vagotomies, bronchial surgeries, hysterectomies, nephrectomies, lysis of adhesions, tumor extraction, knee arthroscopies, and abdominal explorations; microsurgery, i.e. vitreoretinal, otologic, laryngeal and stereotactic procedures; intubations, including neonatal

-8-

procedures; and arterial and venous replacement and bypass methods used, for example, in treatment of innominate and subclavian occlusive disease.

5       The apparatus can be used to provide realistic simulations of patients on which to practice medical procedures for training and qualification purposes, to provide a means for trainees to see and feel actual (or simulated) surgeries, to display information from previously obtained medical diagnostics or image modalities (CT data, PET data, MRI data, etc.) to the surgeon  
10       overlaid on current image information during the surgery, and to provide the man-machine interface for robotic surgery.

15       The apparatus consists of a two or three dimensional display device, a two or three dimensional sound device, a graphics/image processing engine and storage module capable of real-time medical image generation, and programmable tactile/force reflecting mechanisms which can generate the "feel" of medical  
20       instruments and the interaction of these instruments with the anatomical simulation. The preferred embodiment of the invention is designed for simulating endoscopic medical procedures due to the minimally invasive nature of these techniques.

25       The preferred embodiment of this invention addresses the problems presented by the prior art by providing means for controlled, preprogrammable simulation of a medical procedure (using both active tactile feel and imagery) so that standardized practice and  
30       qualification sessions can be performed by surgeons. The same embodiment can also be used to augment the data

-9-

normally delivered to the surgeon in actual endoscopic surgery, and can provide surrogate feels and imagery to surgeon trainees from actual surgeries being performed by expert surgeons.

5           The basic medical procedure simulation system consists of two basic functions:

(1) measuring and recording sights, sounds, and feels generated during actual surgery;

10           (2) accurately playing back these recorded sights, sounds, and feels and for using the recorded data to generate new information necessary to emulate the responses to alternative actions taken by a surgeon trainee.

15           Turning now to Figure 2, the recording apparatus 20 that allows the critical events in a medical procedure to be measured and recorded during actual surgeries performed by expert surgeons is shown. Medical instruments 16 having pressure and position sensors 22 are connected to a data digitizer 24. The pressure and position data from the digitizer 24 is recorded by a recording system 26 consisting of a computer and a storage subsystem. A viewing scope 14 having pressure and position sensors 28 is connected to an image digitizer/recorder 30. The image digitizer/recorder 30 is also connected to the recording system 26. The recording system 26 can either compress and store digital image data or store analog video on a computer-controlled video cassette recorder (VCR). The non-image data is stored on digital disk or tape storage. An accurate time base 32 is also connected to the recording subsystem 26 to provide time stamps for the instrument locations, forces or pressures, and

20  
25  
30

-10-

actions such as trigger actuations during the specified scope locations, forces (or pressures), and image data captured during the operation. Each data item (force, position, trigger action item or image captured) is time stamped so that it is placed accurately into the time sequence of events during surgery. The recording apparatus 20 in Figure 2 can be directly connected to a playback apparatus (in Figure 5) to provide immediate feedback to a trainee.

10 To support the generation of data and images to accommodate various user inputs, which will be different than the mechanics implemented in the operating room and will differ from any particular surgery performed, a systematic scanning of anatomical features is performed. Figure 3 depicts the systematic scanning of anatomical features using the scope 14 to generate a complete imagery record of organ and tissue orientation surrounding the site of medical simulation. This supports generation of in-between data and interpolated views based on recorded data.

The virtual reality training/replay apparatus 40 needed to playback the recorded data is incorporated in Figure 4. This apparatus 40 generates the virtual space which displays the time stamped and interpolated data stored in the image and data storage system 42. A virtual reality control computer 44 receives image and non-image data from the image and data storage system 42. Position, orientation, and force data are processed by the computer 44 and sent to the force/tactile programmed controller and hand/instrument tracking subsystem 46. The force/tactile programmed controller and hand/instrument tracking subsystem 46 is connected to a

-11-

tactile/force reflecting subject simulation mechanism 48 in order to provide force feedback.

5           The virtual reality control computer 44 obtains image data from the image and data storage system 42 based on the position and orientation of the instruments. The control computer 44 processes this data and relays it to an image warp processor 50. The image warping function 50 uses morphing, defined as the correspondence of two images through corresponding  
10       polygon patches, as the means for providing interpolated images from data collected during recording sessions. A 3D graphics generator 52 is also connected to the virtual reality control computer 44 in order to generate accurate three dimensional images of endoscopic instru-  
15       ments. A graphics overlay unit 54 is used to overlay the three dimensional images from the 3D graphics generator 52 on the morphed video derived imagery from the image warp processor 50. The output of the graphics overlay unit 54 is fed into a three dimensional display  
20       system 56.

          An optional (denoted by the dashed lines) trainee head tracking system 58 can be connected to the virtual reality control computer 44 to provide information for the three dimensional display generation  
25       function to control generation of view dependent imagery assuming that the display system 56 is a head mounted system. Alternative embodiments for the display system 56 which use more conventional display technology, such as CRTs, might not require head tracking systems 58.  
30       However, future systems are expected to replace CRT viewing of endoscope-derived image data with head-mounted three-dimensional viewing. This viewing ar-

-12-

rangement will require the head position sensing subsystem 58.

5       The inclusion of a head position sensing subsystem 58 also allows the incorporation of a three-dimensional sound generation system 60. The sound generation system receives audio information from the virtual reality control computer 44 and sends this information to a sound system 62. The use of sound generation is also optional since it is not necessary in  
10       simulating endoscopic procedures.

      Figure 5 shows how the recording apparatus 20 in Figure 2 can be used to acquire image and manipulation data 70 which is then used to compose simulation data sets 72 for replay on the virtual reality replay apparatus 40 from Figure 4. An experienced surgeon 74  
15       performs an actual endoscopic medical procedure using endoscopic instruments 76. The recording system 20 is used to measure and record the sights, sounds, feels, and actions occurring during the actual medical procedure. The sights, sounds, feels, and actions data are  
20       stored in the measured data and image storage system 70. Simulation data sets 72 are formed off-line from the measured data 70 by a data composition system 78. The virtual reality training system 40 uses images and data  
25       in the simulation database 72 to allow a trainee 80 to explore this data. The trainee 80 can view, hear, and feel operations through manipulation and positioning of the simulated instruments, or based on his head location. Images or data not in the simulation database 72  
30       are generated through interpolation between images/data items which are in the database 72 (interpolation

-13-

between images is accomplished through morphing -- mapping predetermined image polygons between images).

Figure 5 also shows how the recording apparatus 20 can be used to pick-up data and imagery from an in-progress medical procedure for immediate replay on the virtual reality replay/training apparatus 40. In this mode, the virtual reality replay apparatus 40 immediately receives the output of the recording apparatus 20 via a communications channel 82. Therefore, the trainee 80 does not explore the input data and imagery through manipulation, but rather experiences the data stream. This data includes the virtual forces generated by the force/tactile subsystem and applied to the trainee's hands through the simulated instruments. Thus, the trainee 80 can gain intuitive understanding of the medical procedure, including the feelings, sights, and sounds of the operation, without the risks and possible complications associated with medical intervention.

Figure 6 shows how elements of the virtual reality replay system 40 can be used to provide the surgeon 90 with views of preoperative information and imagery 92, such as CT scans and MRI scans, to augment what is available now for endoscopic procedures (for instance, video imagery from the laparoscope). A surgeon 90 performs an actual medical procedure using endoscopic instruments 94. The recording system apparatus 20 is used to measure and record the actions and images in the instruments 94 during the procedure. The virtual reality training system 40 incorporates pre-operative test data and images 92 with the output of the recording apparatus 20. The use of virtual reality

-14-

display techniques allows metabolic and anatomical structure graphics to be overlaid on the basic video imagery now available to the surgeon 90 -- this is especially valuable if we provide the surgeon 90 with a three dimensional viewer (such as a head-mount three-dimensional viewer) for graphically enhanced anatomical information.

Figure 7 shows how the virtual reality systems described already can also be used to provide feedback from and control information to robotic endoscopic medical equipment 100. A remote surgeon's 102 instruments, viewing scope, and head position are measured and recorded by the virtual reality training system 104. This data is transmitted to the robotic endoscopic surgery equipment 100 via a communications channel 106. A local surgeon's 108 instrument, scope, and head position is also measured and recorded by a second virtual reality training system 110. The robotic instruments are controlled to perform the actions of either the remote surgeon 102 or the local surgeon 108 on the patient 112. The resulting sights, sounds, actions, and feels are experienced by both the remote surgeon 102 and the local surgeon 108. The virtual reality concept described in this document provides the means for sharing control of such robotic equipment 100 between several surgeons or trainees.

The most important subsystems in the virtual reality replay apparatus are the force/tactile controller 46 and the tactile/force reflecting mechanism 48. These systems use force reflection information generated from the simulation database (or model-base) to create the feel of the medical instruments. Figure 8 shows a



-15-

control concept for creating the feel of medical instruments during a simulation. The hands 120 of a surgeon or trainee grasp and move a member representative of an instrument. The position of the instrument 122 is  
5 determined and fed into a geometric model of an organ 124. The geometric model 124 includes data representing the organ size, position, surface characteristics (in terms of elasticity, resistance to searing, slipperiness, etc.). Forces and torques are applied to the  
10 surgeon's/trainee's hands 120 from a force/torque subsystem 126 using data from the geometric model 124. Thus, realistic feels are produced on the simulated medical instrument representing instrument-to-organ interaction forces based on the position of the instrument.  
15

An apparatus for simulating laparoscopic medical procedures shown in Figure 9 uses the servo systems concept described in Figure 8 to provide force-feedback control. The apparatus consists of a  
20 box-like enclosure 130 which provides three openings 132 for insertion of instruments 134. When the instruments 134 are inserted they are clamped to four-axis devices 136 such as the force reflection mechanism 140 shown in Figure 10. This mechanism 140 includes, in effect, a  
25 small backdrivable robot which moves in 4 degrees of freedom: 1 linear position (extension) and 3 attitudes (roll, pitch, and yaw). This is accomplished by the extension actuator 142, roll actuator 144, pitch actuator 146, and yaw actuator 148. This mechanism 140 can  
30 translate and provide forces/torques under programmed control (generated by the modeling subsystem in Figure 8) which feel to the trainee like the interactions characteristic of the actual medical procedure. These

-16-

four-axis actuation systems are reduced implementations of universal force reflection mechanisms described in co-pending application Serial No. 984,324, filed December 2, 1992.

5           In operation, each of the four-axis devices 136 generate a series of signals 139 representative of the position and orientation of the corresponding instrument 134. These signals are transmitted to a controller 138 which generates a series of force com-  
10           mands 137 which are returned to the four-axis devices 136 to provide force feedback on the corresponding instrument 134.

          The controller 138 may be a virtual reality simulation of the environment of a medical procedure,  
15           formed either artificially or based upon data collected during an actual medical procedure. The controller 138 could also represent one or more slave devices which respond to follow the actions of the instruments 134, measure the forces acting on the slave device, and  
20           transmit force commands 137 back to the four-axis devices 136.

          It should be noted that there are a variety of different ways that the four-axis device could be implemented. This device could read the position of a  
25           user's hand by means of a laser tracking system and feedback forces by urging the user's hand with jets of air. In the preferred embodiment, however, the user's hand will grip a member 134 representative of a medical instrument or another medical tool.

-17-

The specific four-axis device shown in Figure 10 is now examined in more detail. The position, orientation, velocity, and/or acceleration provided on the force reflective mechanism 140 by a member 134 is sensed and transmitted as a command to the simulation which implements a virtual reality force field. In turn, a force command is generated based on the force field value for the position, orientation, velocity, and/or acceleration of the member 134 given by the simulation. This force command is transmitted to force reflective mechanism 140. Force is then generated on the member 134 by the force reflective mechanism 140 using four small, brushless, DC servo motors. The four axis force-reflection output and four-axis orientation and position control provides the user with direct kinesthetic feedback from the virtual environment traversed. A queuing button (not shown) can be incorporated in order to actuate the instrument within the simulation or control.

The invention in its preferred embodiment is applicable to controlling a virtual or simulated medical environment. However, the invention is also well suited to the control of a remote or physical medical instrument. Further, the present invention is suited for application to any number of axes. For instance, a full six-axis interface could be used for simulating or controlling medical procedures.

While the best mode for carrying out the invention has been described in detail, those familiar with the art to which this invention relates will recognize various alternative designs and embodiments

-18-

for practicing the invention as defined by the following claims.

-19-

**What Is Claimed Is:**

1. A method for simulating actual medical procedures, the actual medical procedure utilizing at least one medical instrument, the method comprising the steps of:

5 measuring the actions of the medical instrument during an actual medical procedure; and

generating the actions on a member representative of the medical instrument;

10 whereby generating the actions simulates the actual medical procedure.

2. The method of claim 1 further comprising the step of recording the measured actions.

3. The method of claim 2 wherein the step of generating the actions on the member is performed based upon the recorded actions.

4. The method of claim 1 wherein the actual medical procedure includes endoscopic surgery utilizing a viewing scope capable of generating images.

20 5. The method of claim 4 further comprising the step of displaying the generated images.

6. The method of claim 5 further comprising the step of recording the images generated by the viewing scope wherein the step of displaying is performed based upon the generated images as recorded.

7. The method of claim 4 wherein the actual medical procedure includes preoperative exploration with

-20-

the viewing scope and wherein the medical instrument comprises the viewing scope.

8. The method of claim 5 further comprising the step of measuring supplemental information, wherein  
5 the step of displaying is performed in conjunction with the playback of the supplemental information.

9. The method of claim 8 wherein the supplemental information is audio information.

10 10. The method of claim 8 wherein the supplemental information is derived from medical diagnostic equipment.

11. The method of claim 6 wherein the step of displaying is performed based upon diagnostic information.  
15 tion.

12. A system for simulating actual medical procedures, the actual medical procedure utilizing at least one medical instrument, the system comprising:

20 measuring means for measuring the actions of the medical instrument during an actual medical procedure; and

generating means operatively associated with the measuring means for generating the actions on a  
25 member representative of the medical instrument;

whereby the actions of the member simulate the actual medical procedure.

13. The system of claim 12 further comprising recording means operatively associated with the measuring means for recording the measured actions.  
30

-21-

14. The system of claim 13 wherein the generating means is operatively associated with the recording means and wherein the generation of the actions on the member is performed based upon the recorded actions.

15. The system of claim 12 wherein the actual medical procedure includes endoscopic surgery utilizing a viewing scope capable of generating images.

16. The system of claim 15 further comprising display means operatively associated with the viewing scope for displaying the images generated by the viewing scope.

17. The system of claim 16 further comprising recording means operatively associated with the viewing scope and the display means for recording the generated images wherein the display of the generated images is performed based upon the recorded images.

18. The system of claim 15 wherein the actual medical procedure includes preoperative exploration with the viewing scope and wherein the medical instrument comprises the viewing scope.

19. The system of claim 16 further comprising supplemental information means, operatively associated with the display means, for measuring supplemental information, wherein the display of the generated images is performed in conjunction with the playback of the supplemental information.

-22-

20. The system of claim 19 wherein the supplemental information means measures audio information.

5           21. The system of claim 20 wherein the supplemental information means measures information from medical diagnostic equipment.

10           22. The system of claim 18 wherein the display means further comprise means for displaying diagnostic information.

15           23. A method for providing a virtual reality in response to a position and orientation of a member representative of a medical instrument, the method comprising the steps of:

generating an electrical signal for each of a plurality of degrees of freedom of the member as a function of the position and orientation of the member in three-dimensional space;

20           generating at least one virtual reality force field in response to the generated electric signals;

generating a force signal for each degree of freedom as a function of the force field; and

25           directing a force on the member for each force signal, the generated forces providing the virtual reality.

30           24. The method of claim 23 wherein the virtual reality force field is also generated in response to information obtained from an actual medical procedure.



-23-

25. The method of claim 23 wherein the virtual reality force field is also generated in response to information obtained during pre-medical diagnostic procedures.

5           26. The method of claim 23 wherein the generated forces are tactile forces.

27. A method for controlling a medical instrument during a medical procedure, the method comprising the steps of:

10           measuring the position and orientation of a member representative of the medical instrument;

          generating actions on the medical instrument based upon the measured position and orientation of the member;

15           measuring the forces acting upon the medical instrument; and

          generating forces on the member based upon the measured forces on the medical instrument.

20           28. The method of claim 27 wherein the step of measuring the forces acting upon the medical instrument includes measuring torques acting upon the medical instrument.

25           29. The method of claim 28 wherein the step of generating the forces on the member includes generating torques on the member.

30. The method of claim 27 wherein the medical instrument includes an endoscopic medical viewing scope capable of generating images.

-24-

31. The method of claim 30 further comprising the step of displaying the generated images.

32. The method of claim 30 wherein the medical procedure includes preoperative exploration with the viewing scope.

33. The method of claim 31 further comprising the step of measuring supplemental information, wherein the step of displaying is performed in conjunction with the playback of the supplemental information.

34. The method of claim 33 wherein the supplemental information is audio information.

35. The method of claim 33 wherein the supplemental information is derived from medical diagnostic equipment.

36. The method of claim 33 wherein the step of displaying is performed based upon diagnostic information.

37. The method of claim 27 further comprising the step of actuating the medical instrument in response to a command input.

38. A system for controlling a medical instrument during a medical procedure, the system comprising:

first measuring means for measuring the position and orientation of a member representative of the medical instrument;

-25-

first generating means operatively associated with the first measuring means for generating actions on the medical instrument based upon the measured position and orientation of the member;

5           second measuring means for measuring the forces acting upon the medical instrument; and

          second generating means operatively associated with the second measuring means for generating forces on the member based upon the measured forces on the medical  
10   instrument.

39. The system of claim 38 wherein the second measuring means includes means for measuring torques acting upon the medical instrument.

40. The system of claim 39 wherein the second  
15   generating means includes means for generating torques on the member.

41. The system of claim 38 wherein the medical instrument includes an endoscopic medical viewing scope capable of generating images.

20           42. The system of claim 41 further comprising display means operatively associated with the viewing scope for displaying the generated images.

43. The system of claim 41 wherein the medical procedure includes preoperative exploration with  
25   the viewing scope.

44. The system of claim 41 further comprising supplemental information means, operatively associated with the display means, for measuring supplemental

-26-

information, wherein the display of the generated images is performed in conjunction with the playback of the supplemental information.

5           45.    The system of claim 44 wherein the supplemental information means measures audio information.

10           46.    The system of claim 45 wherein the supplemental information means measures information from medical diagnostic equipment.

          47.    The system of claim 43 wherein the display means further comprise means for displaying diagnostic information.

15           48.    The system of claim 38 further comprising actuation means operatively associated with the medical instrument for actuating the medical instrument in response to a command input.

          49.    A system for providing four-axis control for a medical instrument comprising:

20               a member representative of the medical instrument;

              a four-axis device securable to the member, the four-axis device being responsive to the position and orientation of the member to generate electrical signals representative of the position and orientation of the member, the four-axis device including an actuator for each axis of the device;

25               means for actuating the medical instrument in response to the electrical signals;

-27-

means for generating a force field based upon  
a force induced upon the medical instrument; and

means for generating a force signal for each  
axis of the four-axis device as a function of the force  
5 field, wherein the actuators are responsive to their  
respective force signals to provide a force to each axis  
of the four-axis device for reflecting the force on the  
medical instrument to the member;

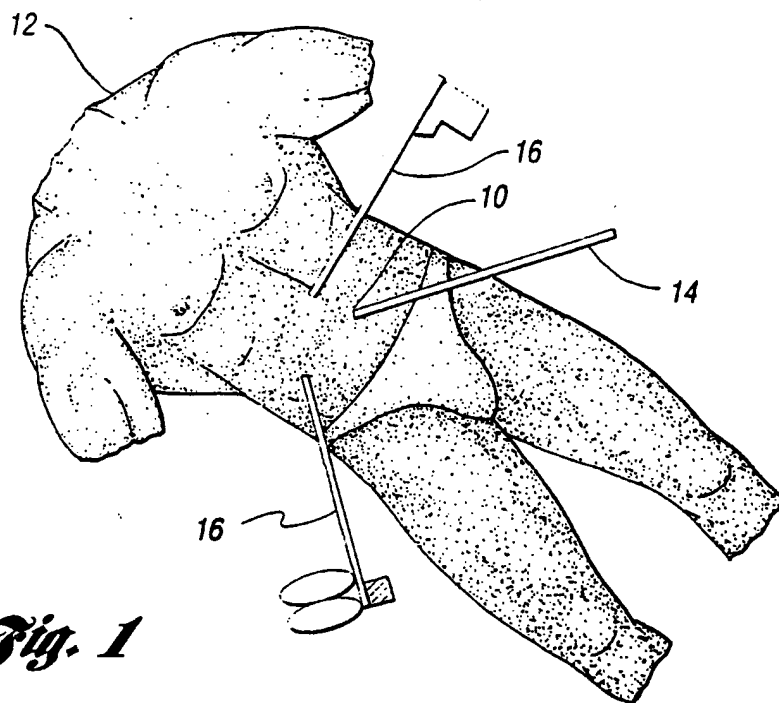
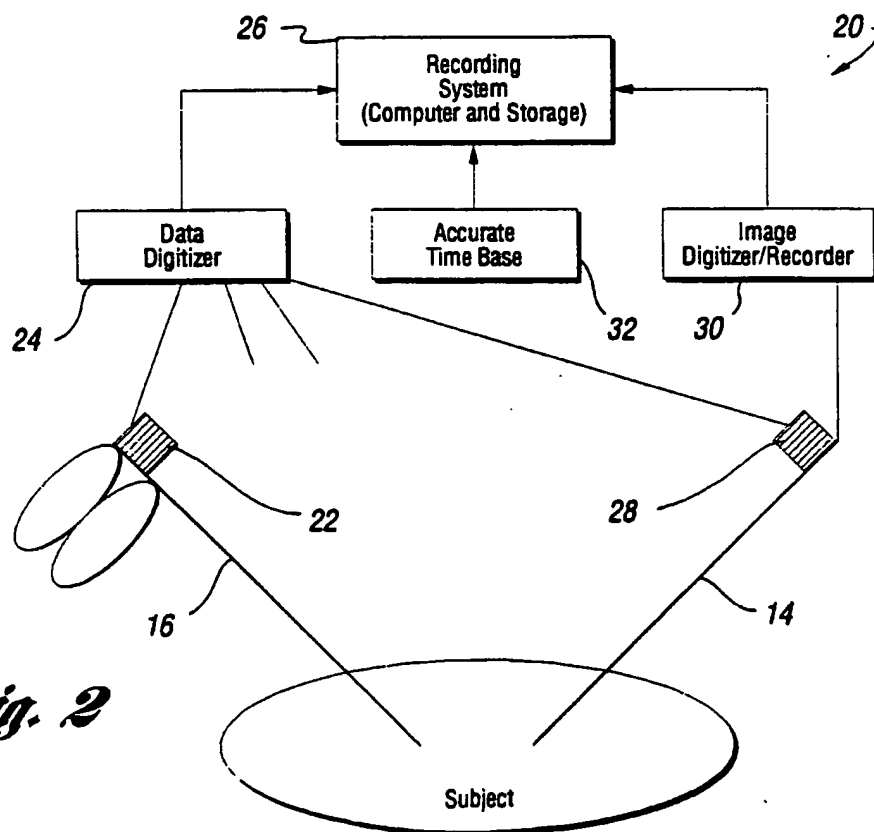
whereby the position and orientation of the  
10 member control the medical instrument.

50. The system of claim 49 wherein the four-  
axis device further comprises an encoder coupled to each  
actuator for generating the corresponding electrical  
signals.

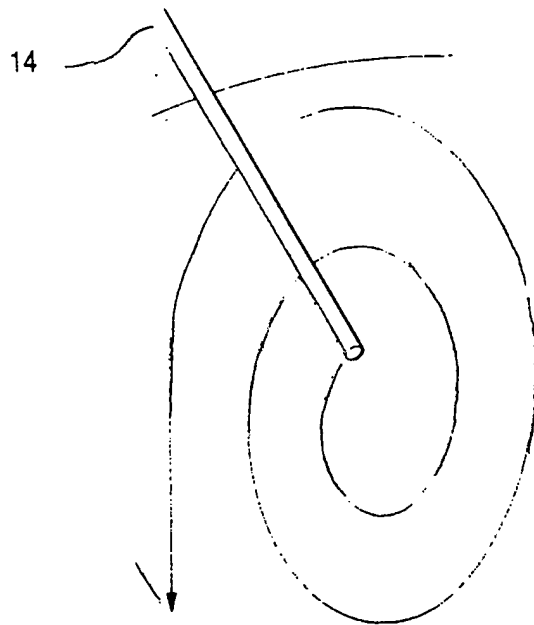
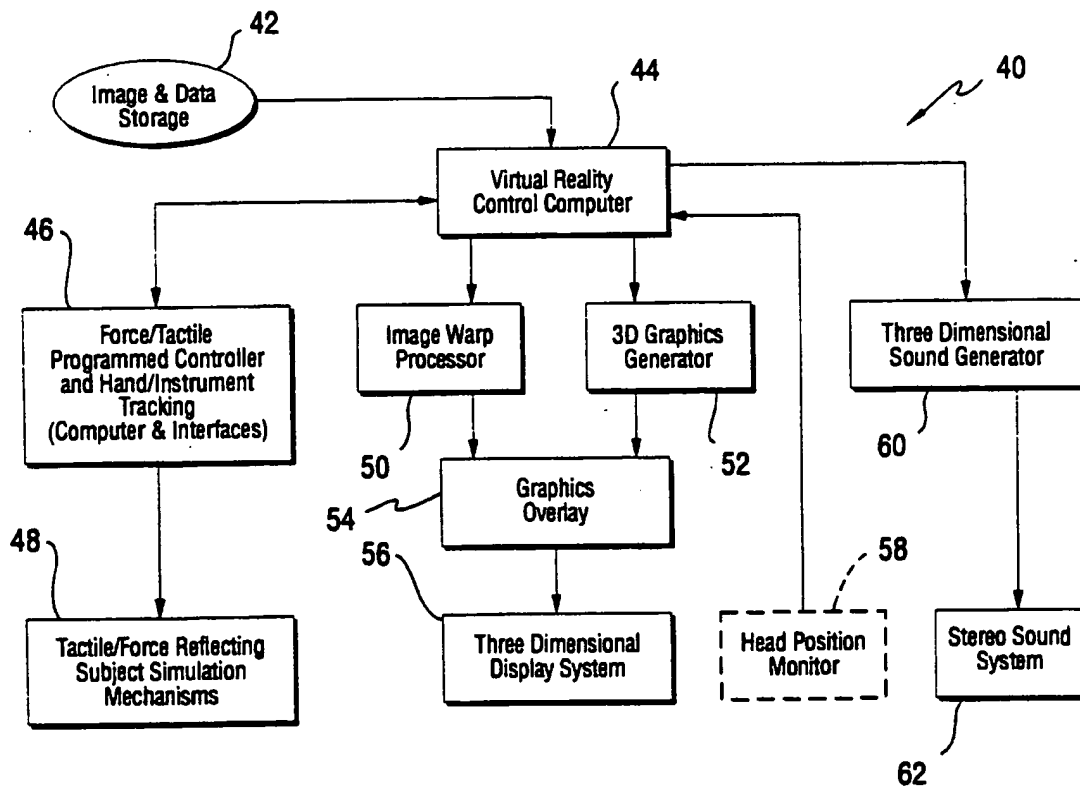
15 51. The system of claim 49 wherein the  
actuators are electric motors.

52. The system of claim 51 wherein the  
electric motors are back-drivable.

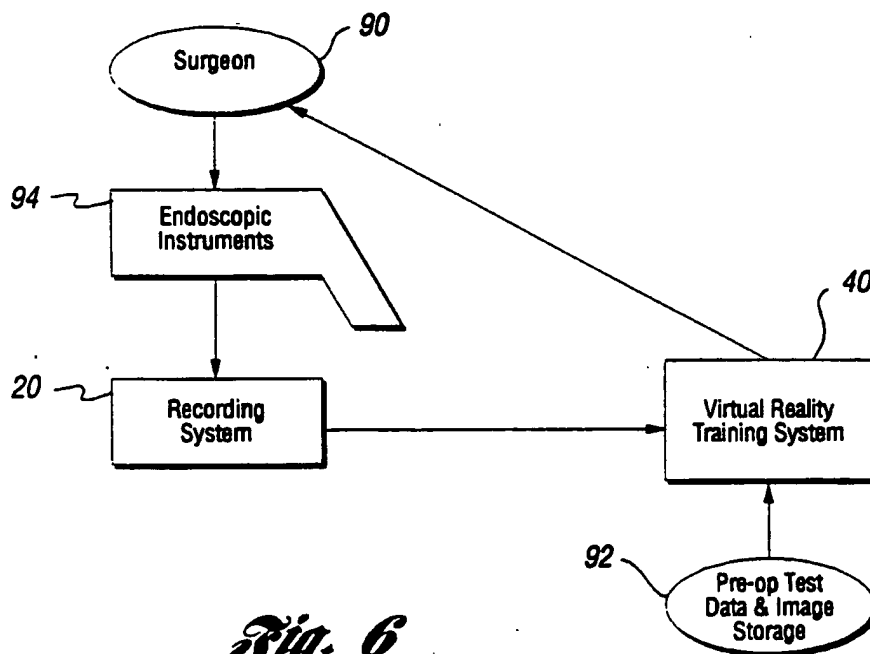
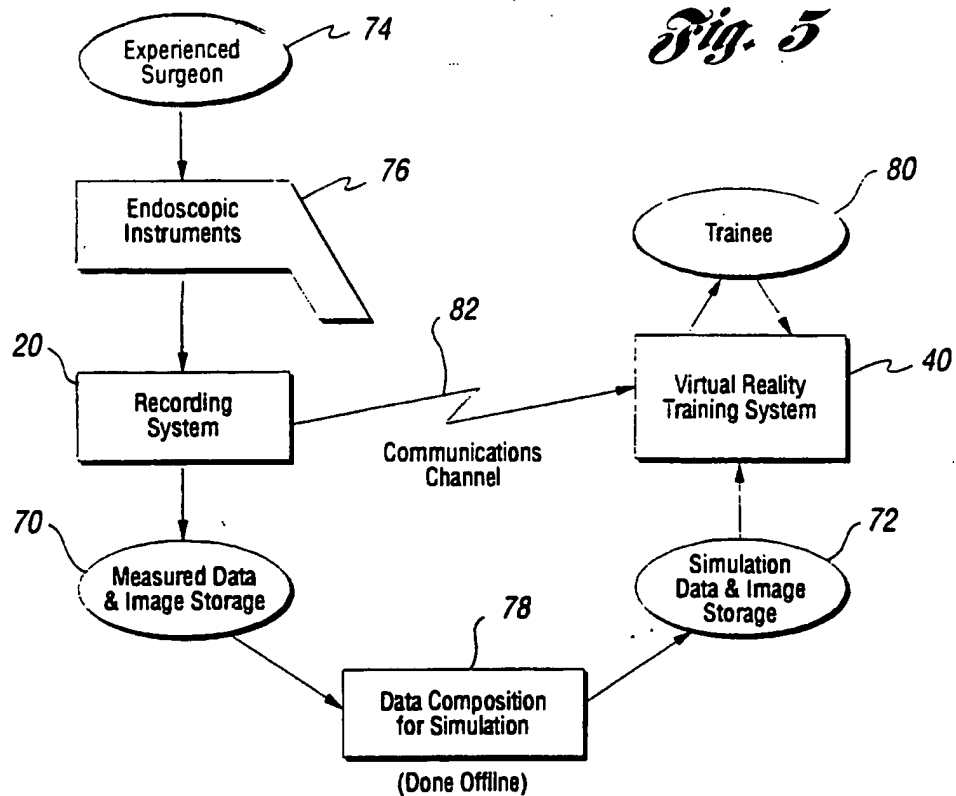
1/5

**Fig. 1****Fig. 2**

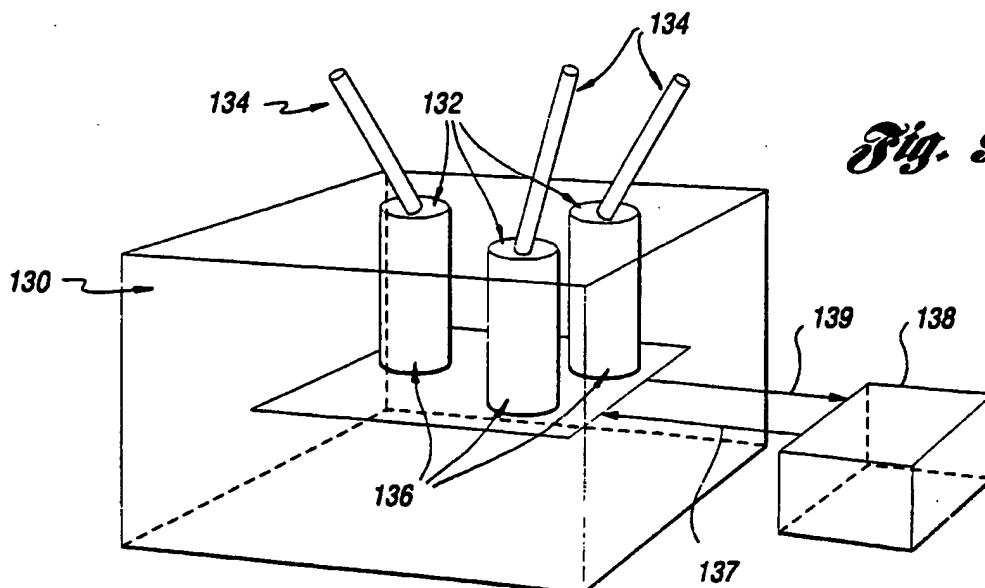
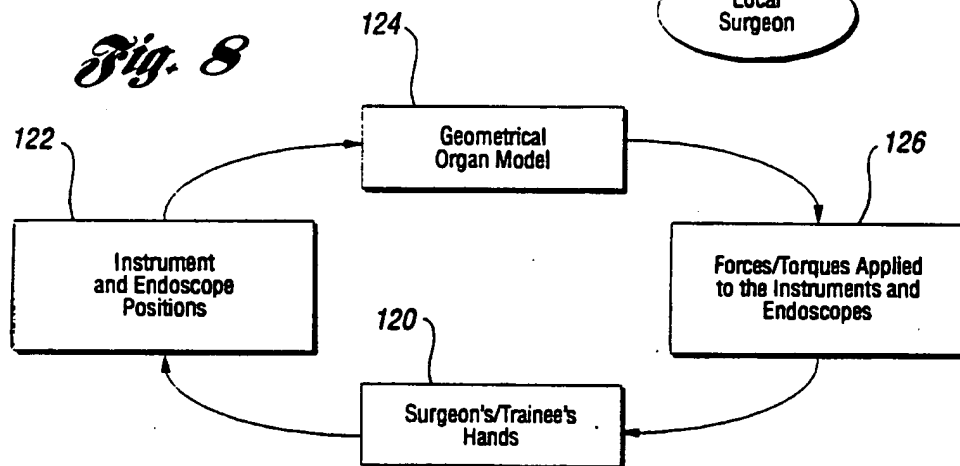
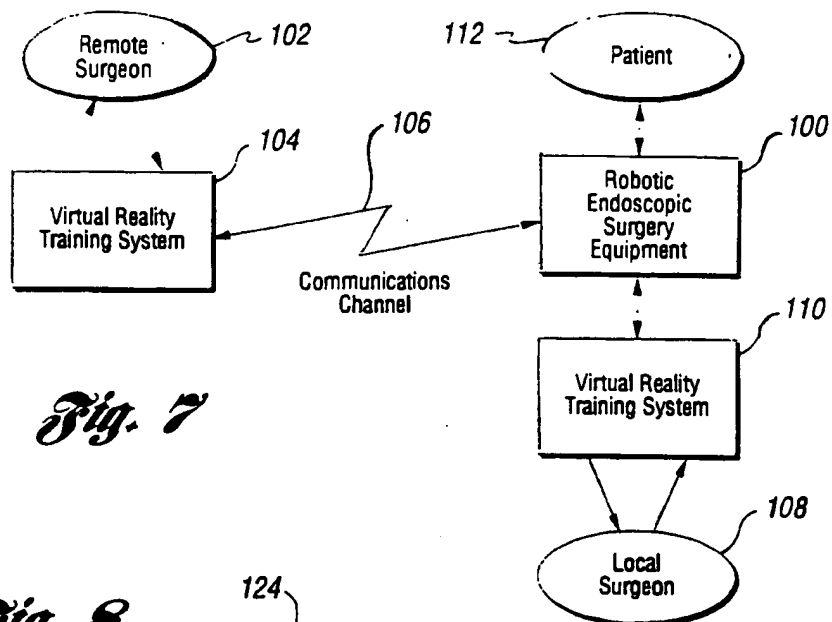
2 / 5

*Fig. 3**Fig. 4*

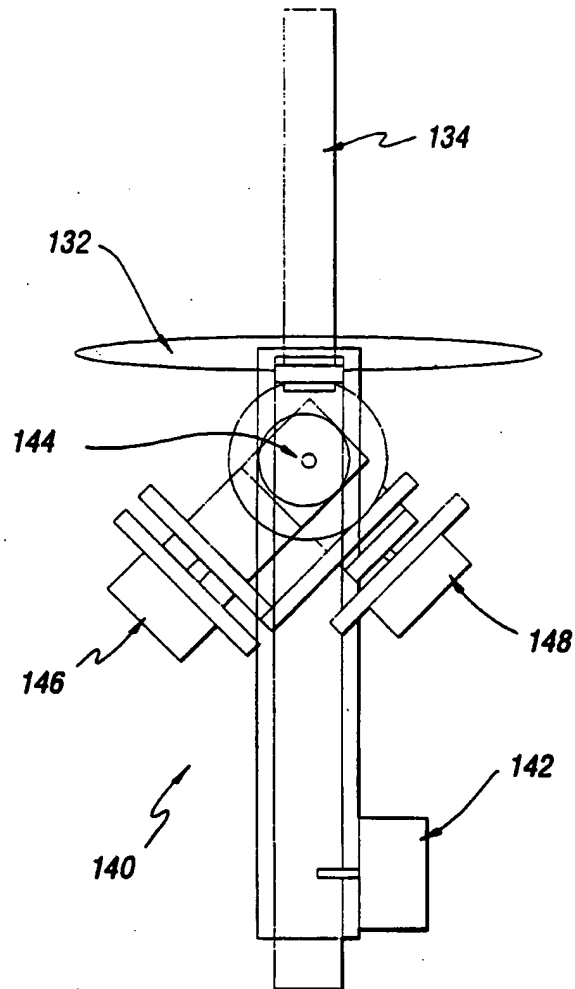
3/5

*Fig. 5**Fig. 6*





5/5

*Fig. 10*

## INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 94/07218

A. CLASSIFICATION OF SUBJECT MATTER  
 IPC 6 G09B23/28 A61B1/00 A61B19/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 G09B A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	GB,A,2 187 101 (NINAN, CHAMPIL ABRAHAM; US) 3 September 1987 see page 1, line 90 - page 4, line 82; claims 1-11	1-3, 12-15
A	---	23-25, 27, 38
Y	DE,A,42 13 584 (OLYMPUS OPTICAL CO.) 5 November 1992 see column 4, line 11 - column 14, line 24; claims 1-23; figures 1-21	1-3, 12-15 4-7, 16-18, 23-25
A	---	
	--- -/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

## \* Special categories of cited documents:

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \*Z\* document member of the same patent family

Date of the actual completion of the international search

6 October 1994

Date of mailing of the international search report

17. 10. 94

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
 NL - 2280 HV Rijswijk  
 Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
 Fax (+31-70) 340-3016

Authorized officer

Gorun, M

## INTERNATIONAL SEARCH REPORT

Inter:      nal Application No

PCT/US 94/07218

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	EP,A,0 391 376 (DANON,NISSIM NEJAT; IL) 10 October 1990 see column 4, line 31 - column 19, line 4; claims 1,2,5,7-11,14-29	1-3, 12-15
A		4-7, 16-18, 27-32, 38-43, 49,51
P,Y	EP,A,0 571 827 (IBM) 1 December 1993 see column 5, line 18 - column 22, line 43; claims 1-26	1-3, 12-15
A	US,A,4 907 973 (HON,DAVID C.;US) 13 March 1990 see column 4, line 28 - column 15, line 34; claims 1-42	1-7
A	PEDERSEN,PEDER C. 'PROCEEDINGS OF THE 12TH ANNUAL INTERNATIONAL CONFERENCE OF THE IEEE ENGINEERING IN MEDICINE AND BIOLOGY SOCIETY' 1 November 1990 , IEEE , PHILADELPHIA VOL.12,PART 1,MAZIER B. et al. "Computer Assisted Interventiopnist Imaging: Application to The Vertebral Column Surgery" pages 430-431 see the whole document	1,12,13, 27
A	WO,A,92 16141 (WILK,PETER J.;US) 1 October 1992 cited in the application see the whole document	1,27, 29-32, 37-43

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 94/07218

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
GB-A-2187101	03-09-87	US-A- 4742815 DE-A- 3700082 JP-A- 62170223	10-05-88 03-09-87 27-07-87
DE-A-4213584	05-11-92	JP-A- 4325147	13-11-92
EP-A-0391376	10-10-90	US-A- 5049147	17-09-91
EP-A-0571827	01-12-93	JP-A- 6030896	08-02-94
US-A-4907973	13-03-90	AU-A- 4517789 CA-A- 2002919 EP-A- 0426767 JP-T- 6506301 WO-A- 9005971	12-06-90 14-05-90 15-05-91 14-07-94 31-05-90
WO-A-9216141	01-10-92	US-A- 5217003 US-A- 5217453 AU-A- 1675392	08-06-93 08-06-93 21-10-92